





1/18

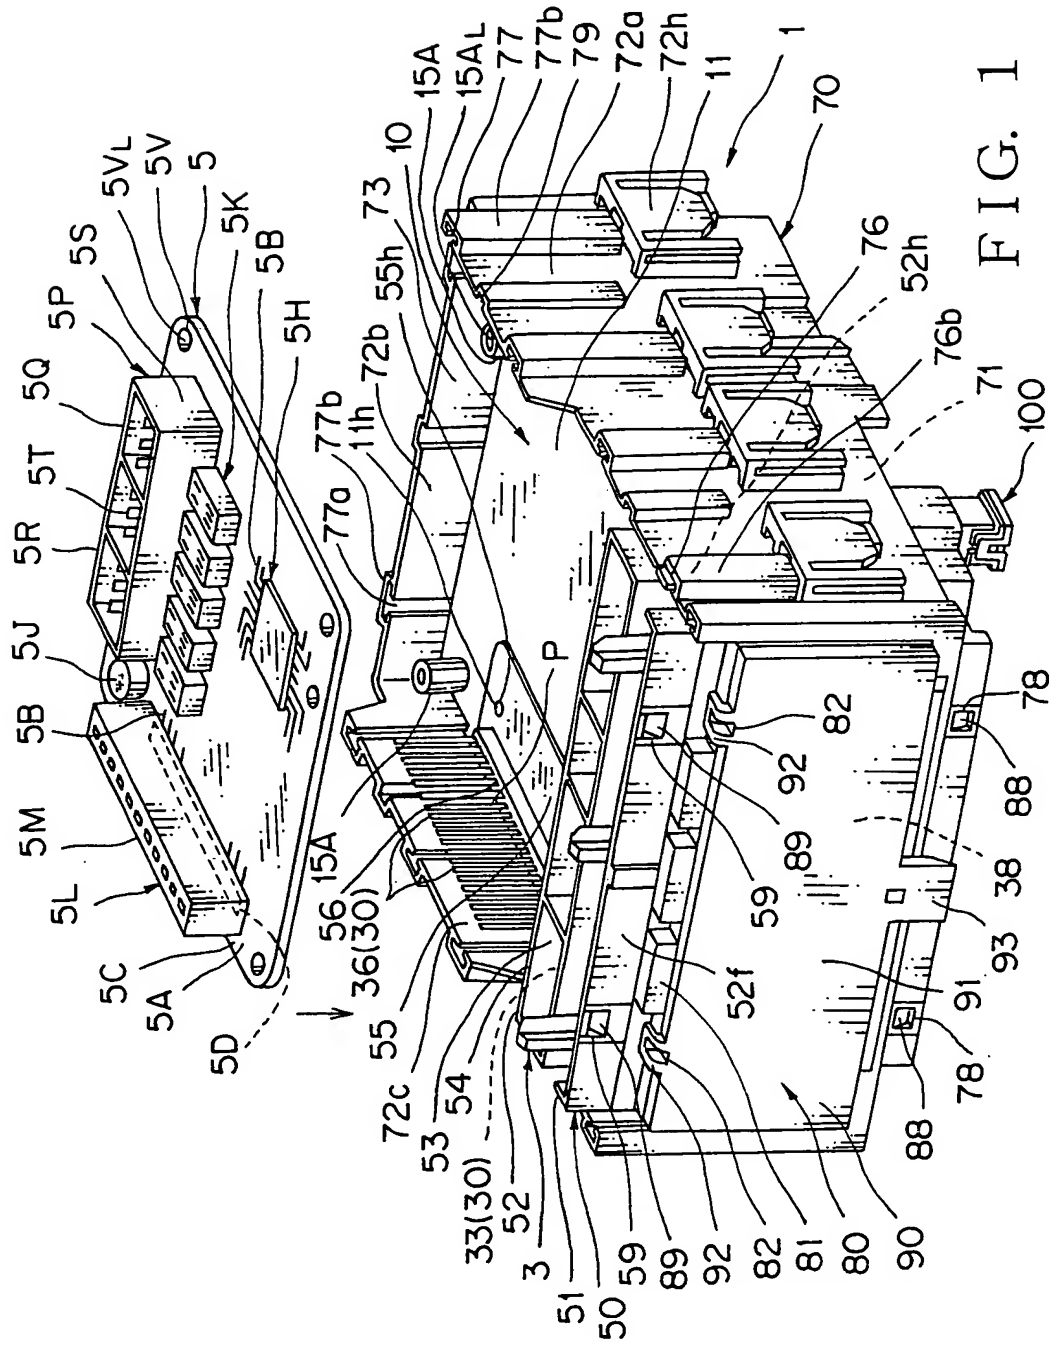

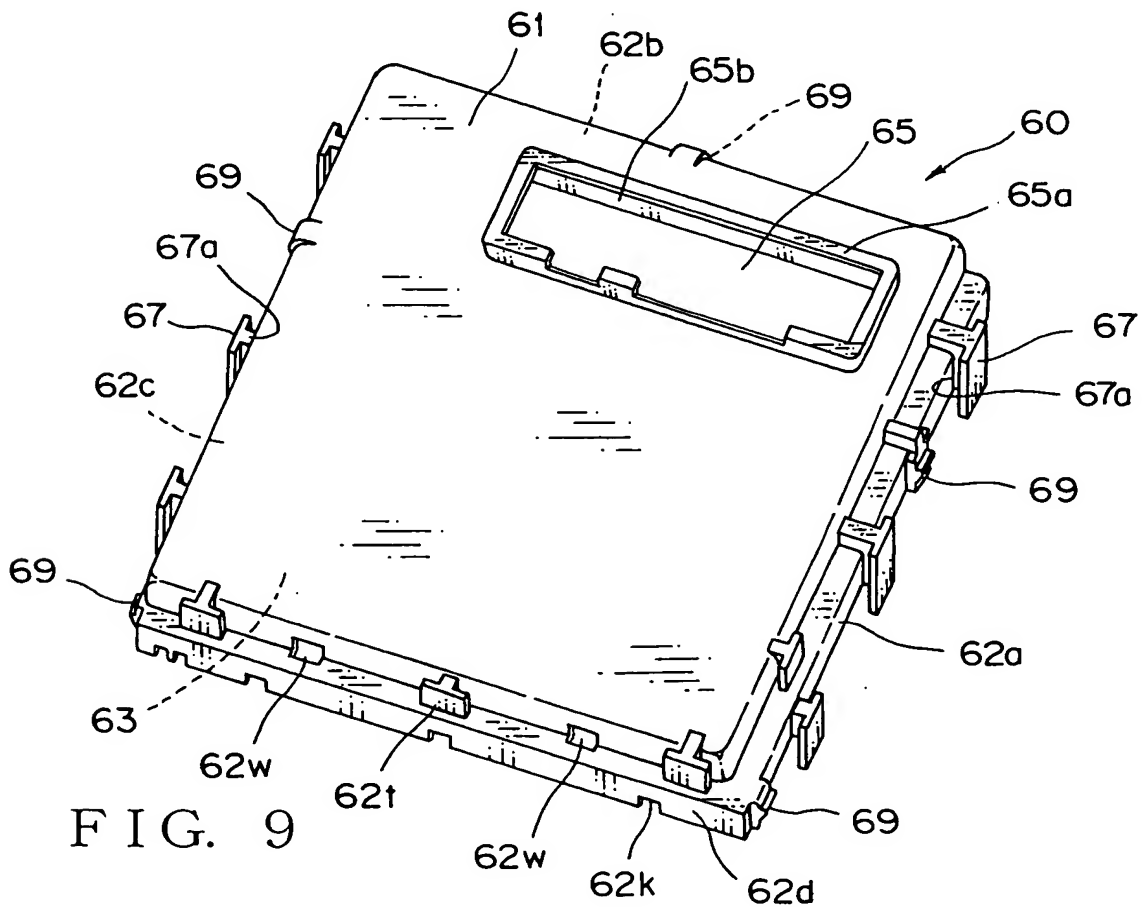

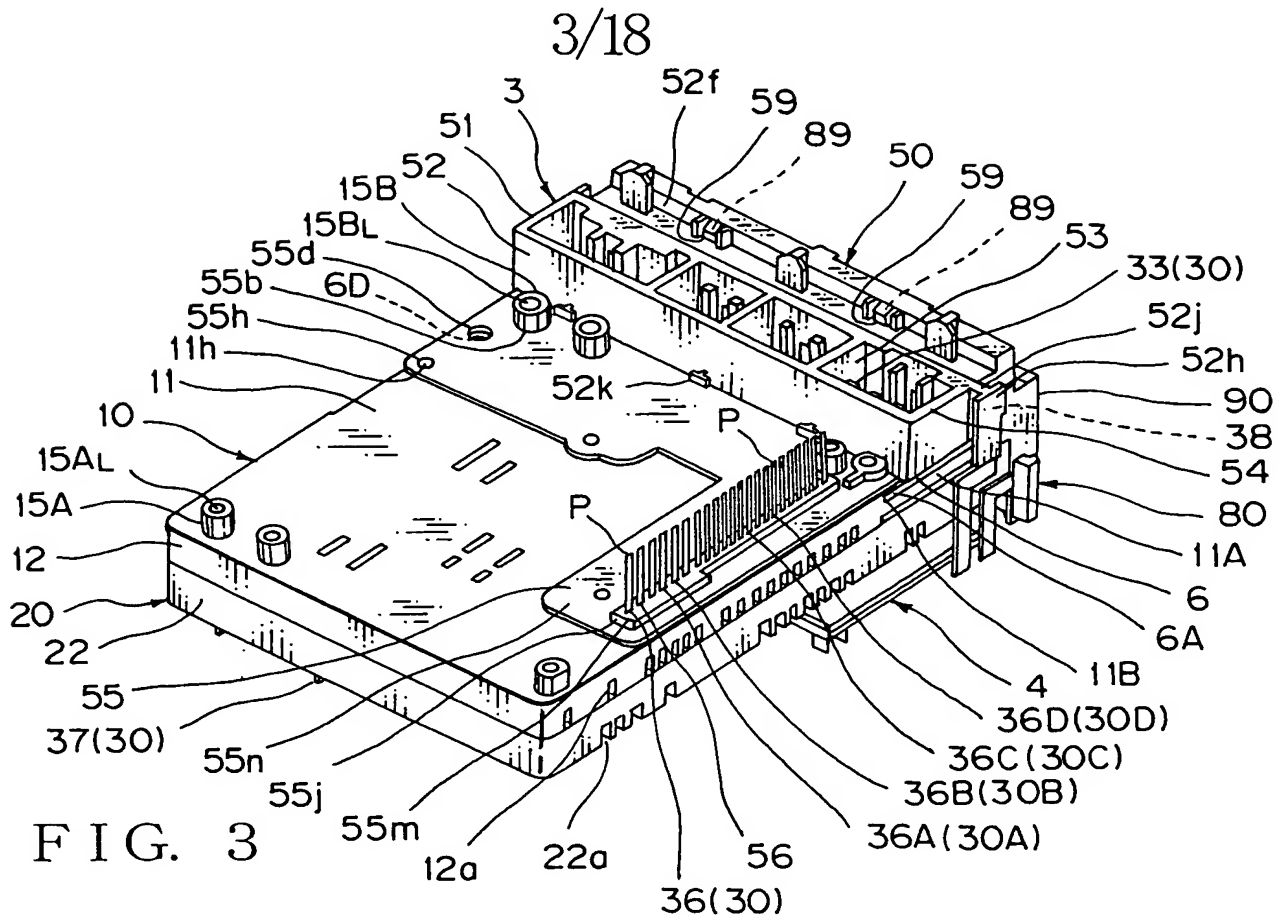

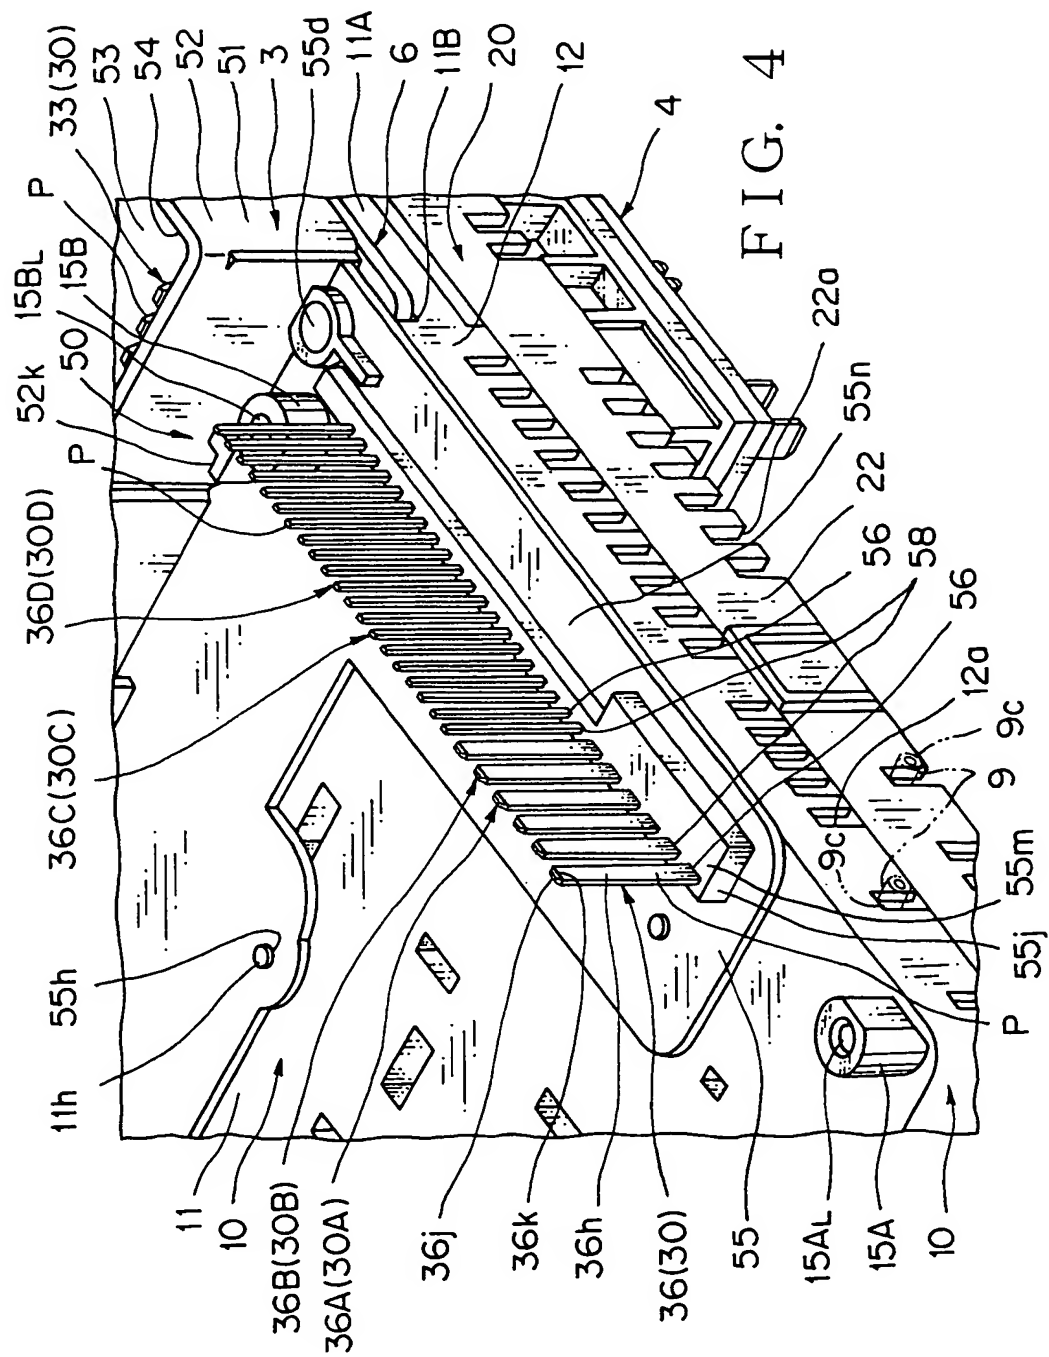

5/18

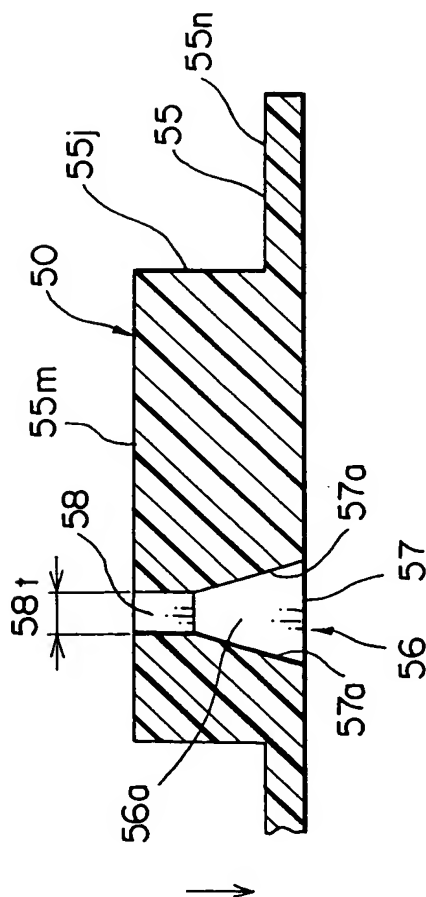


FIG. 5



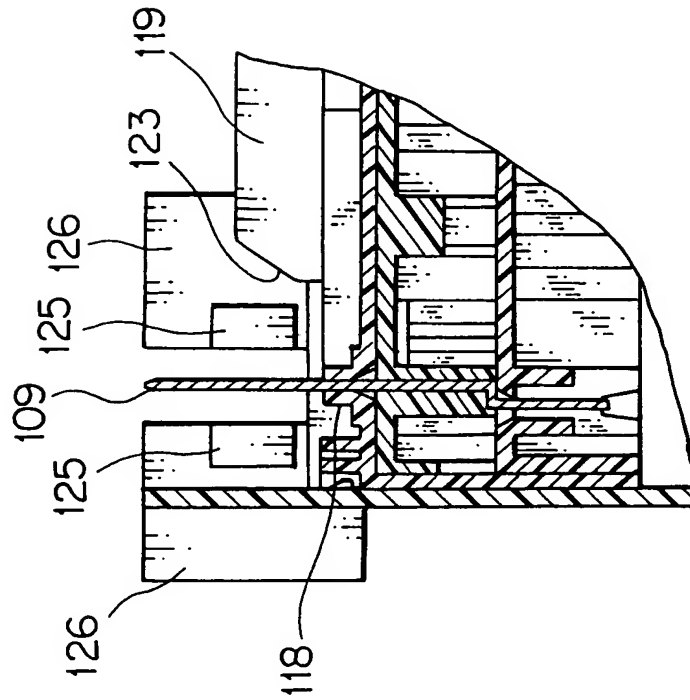


FIG. 15

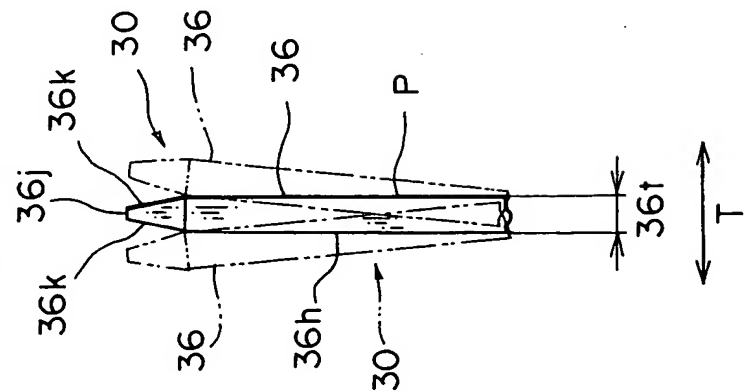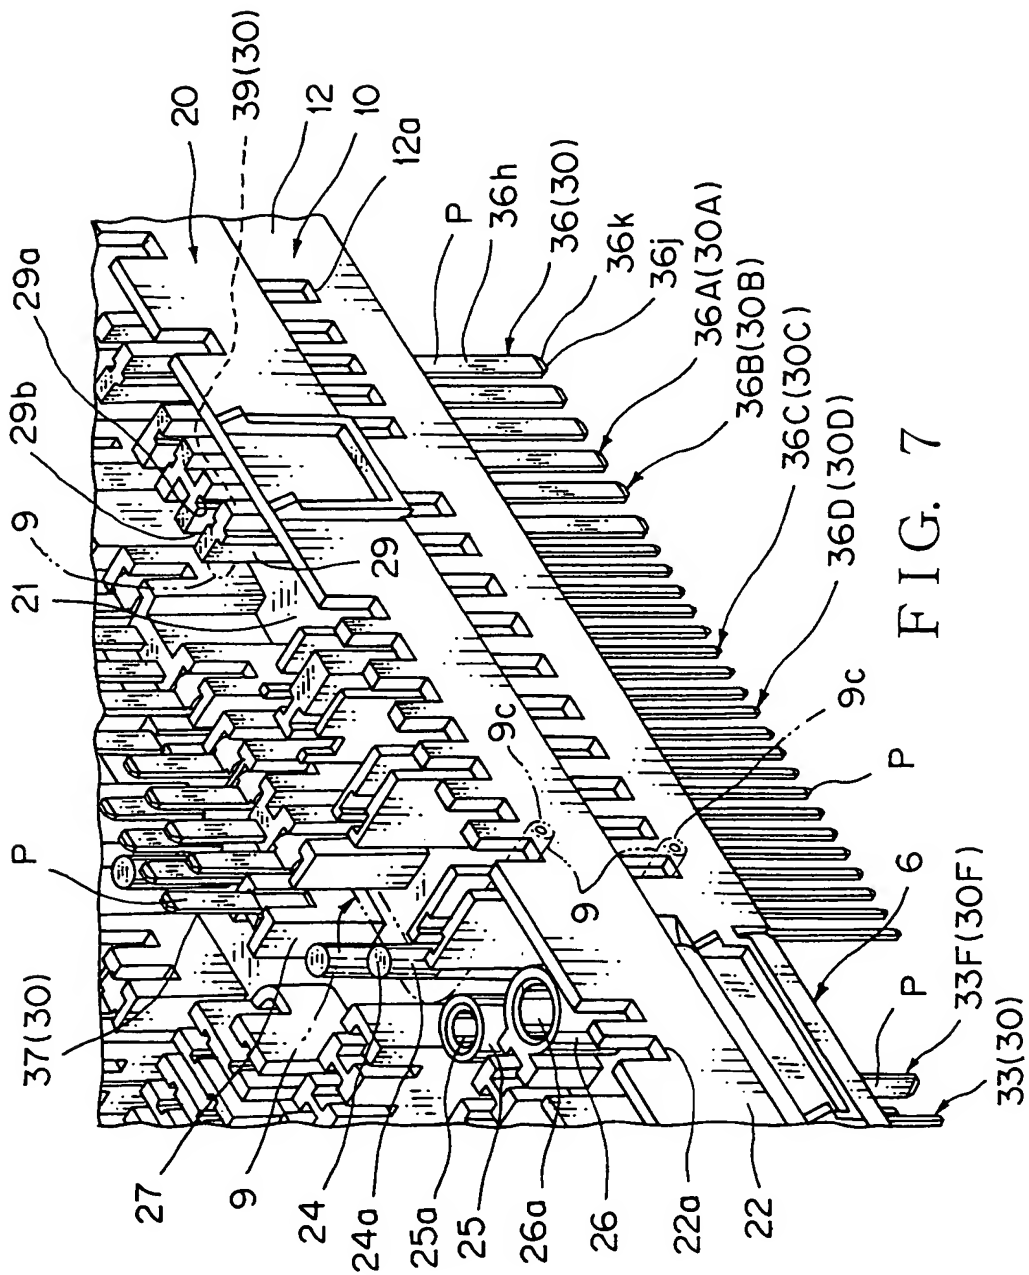

8/18

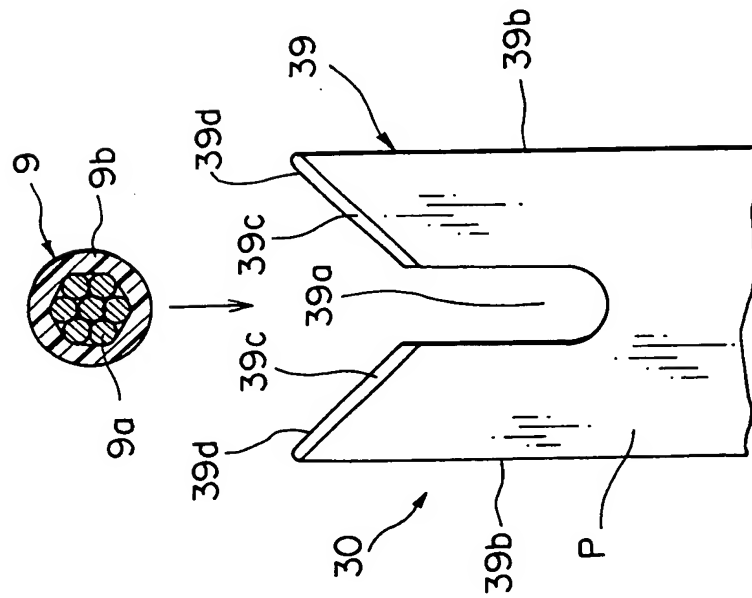


FIG. 8A




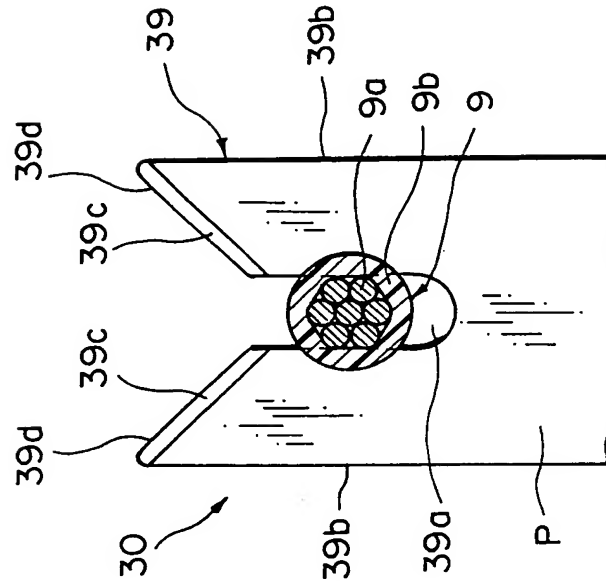


FIG. 8B


9/18

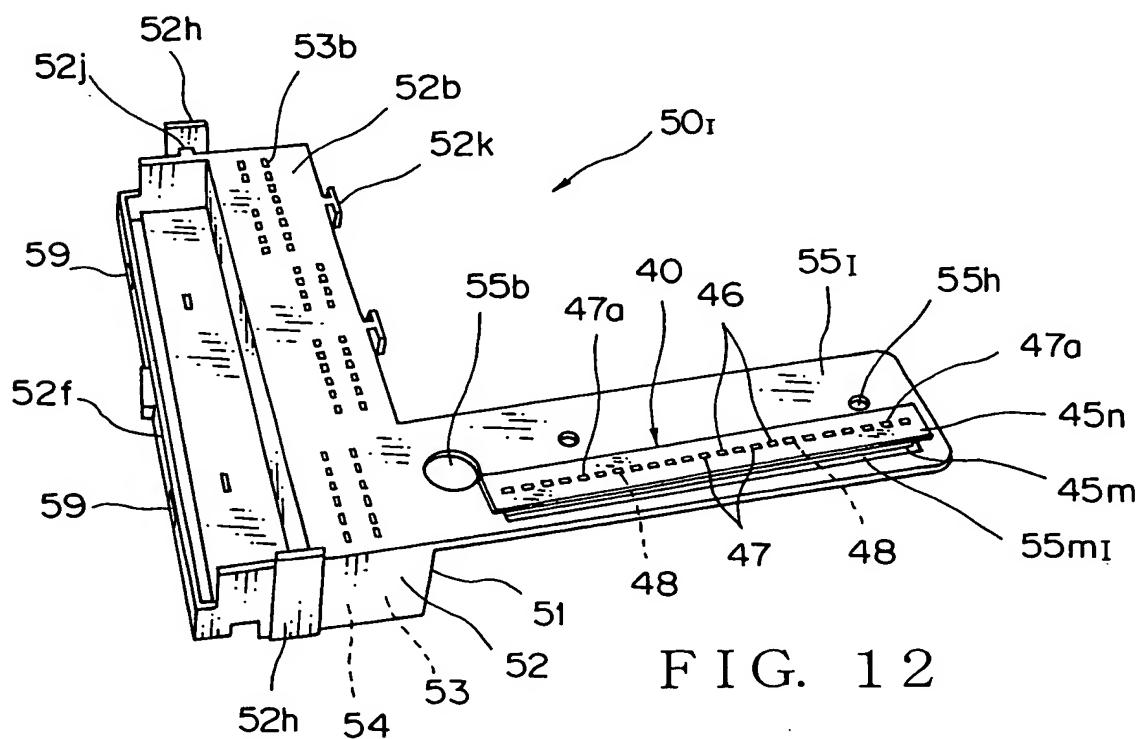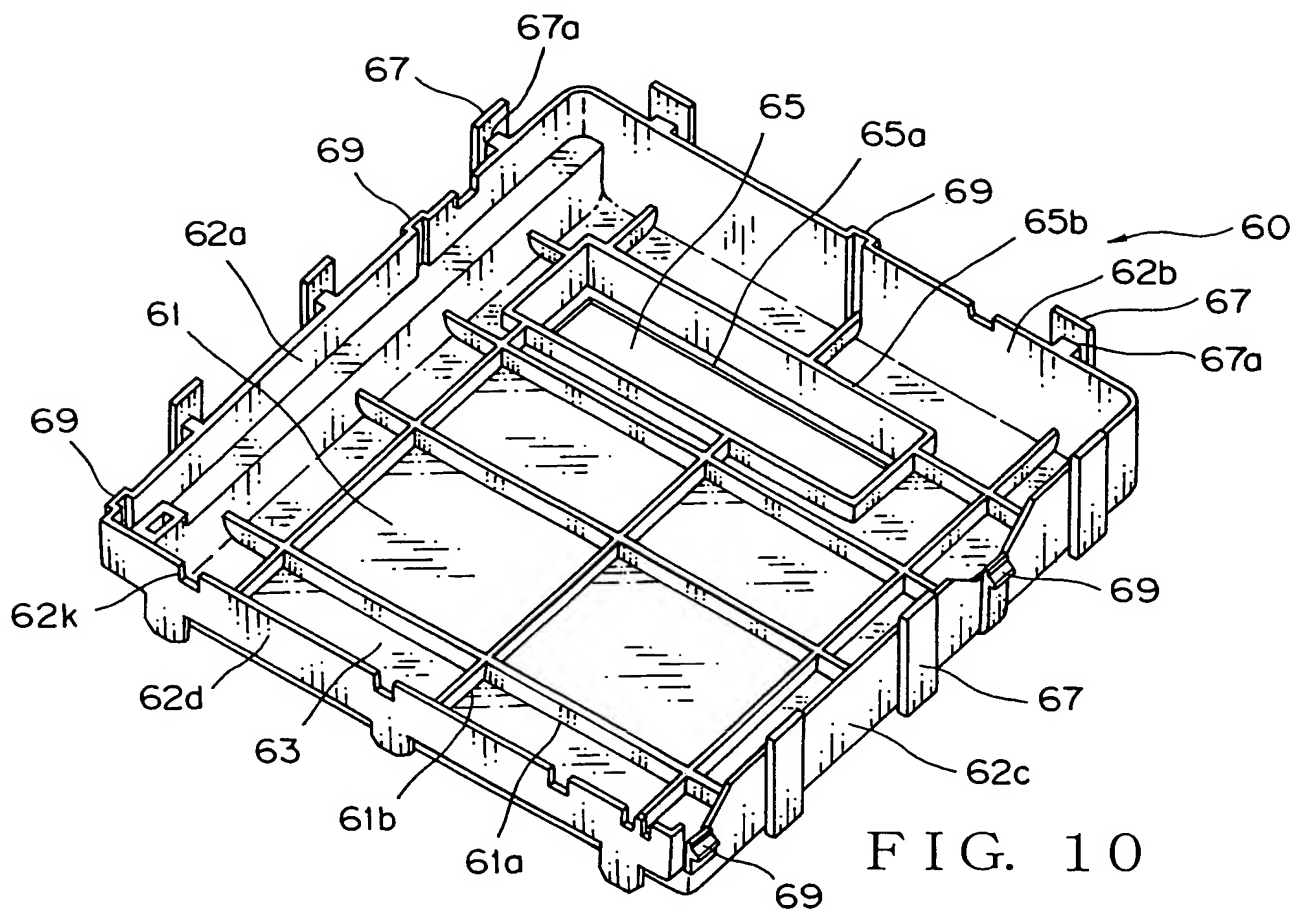



10/18

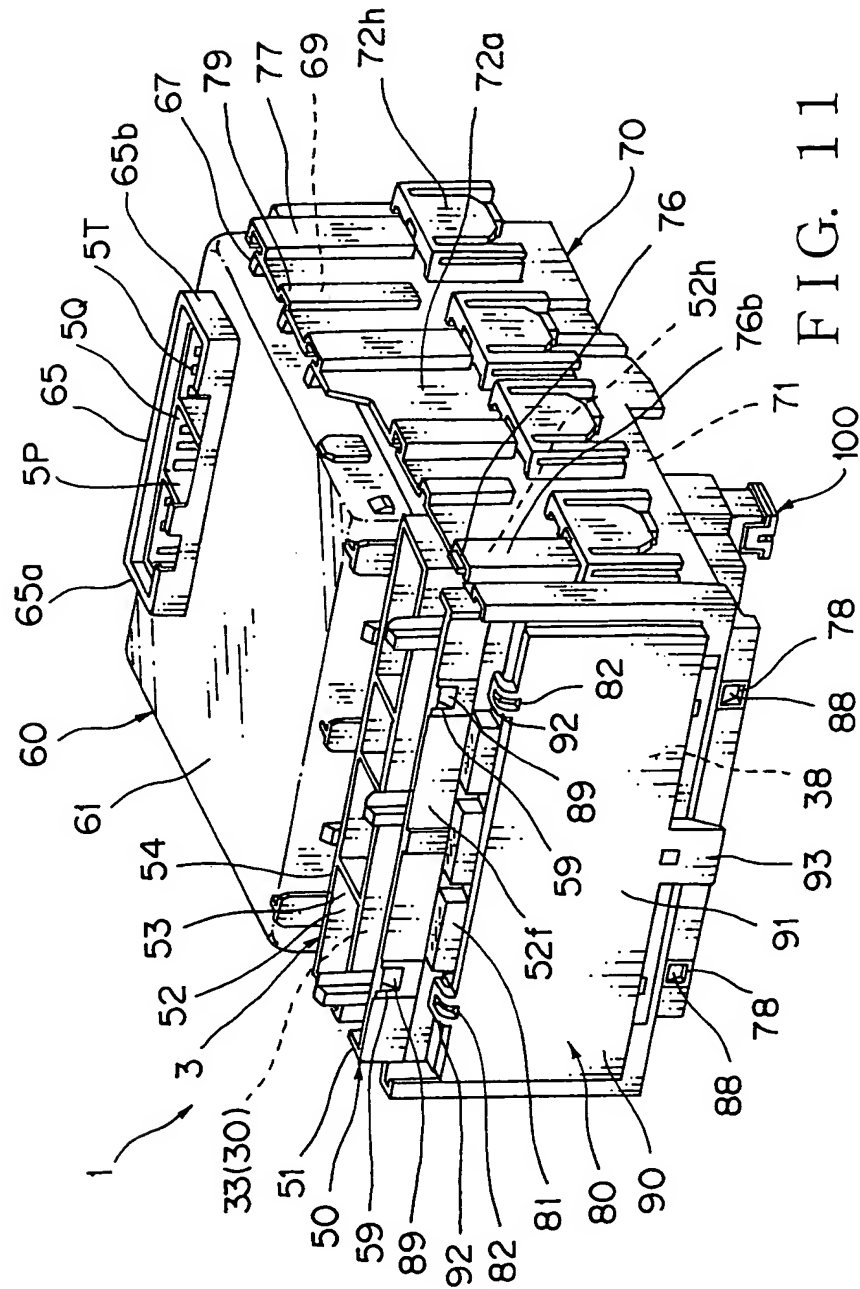

11/18

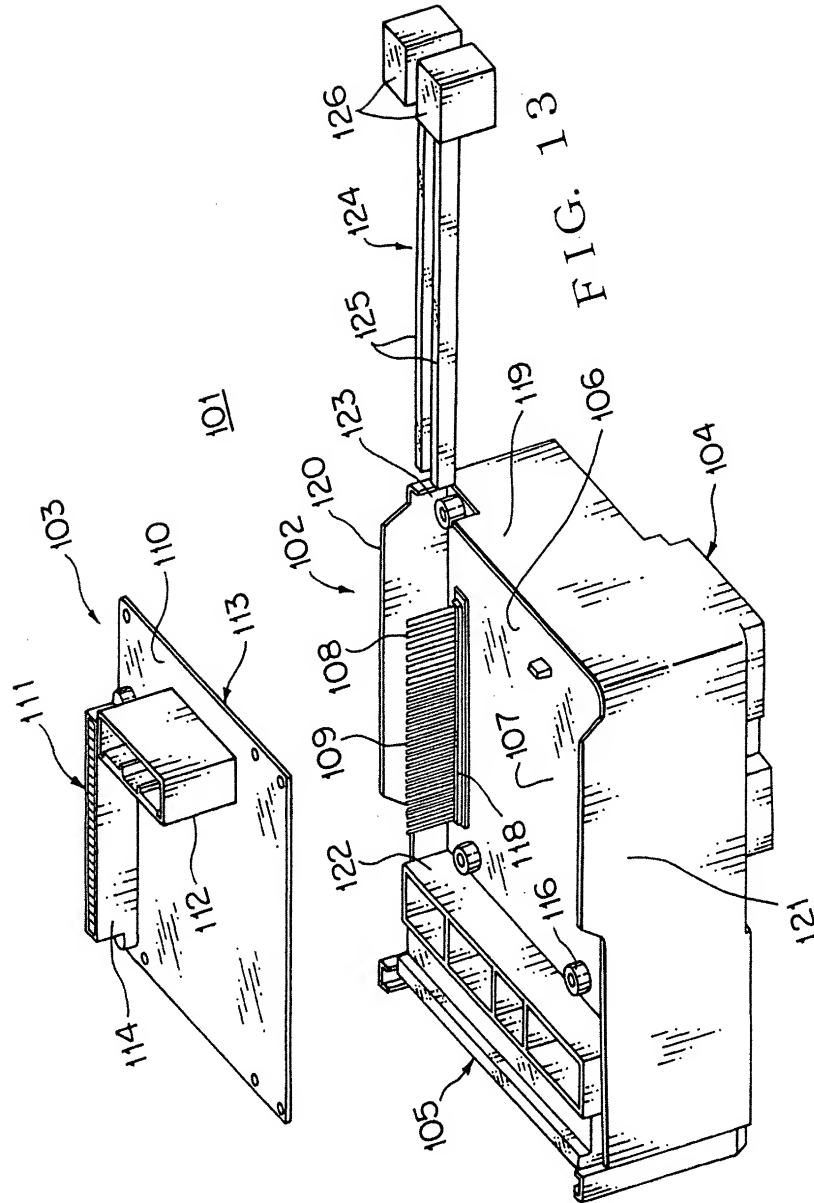

12/18

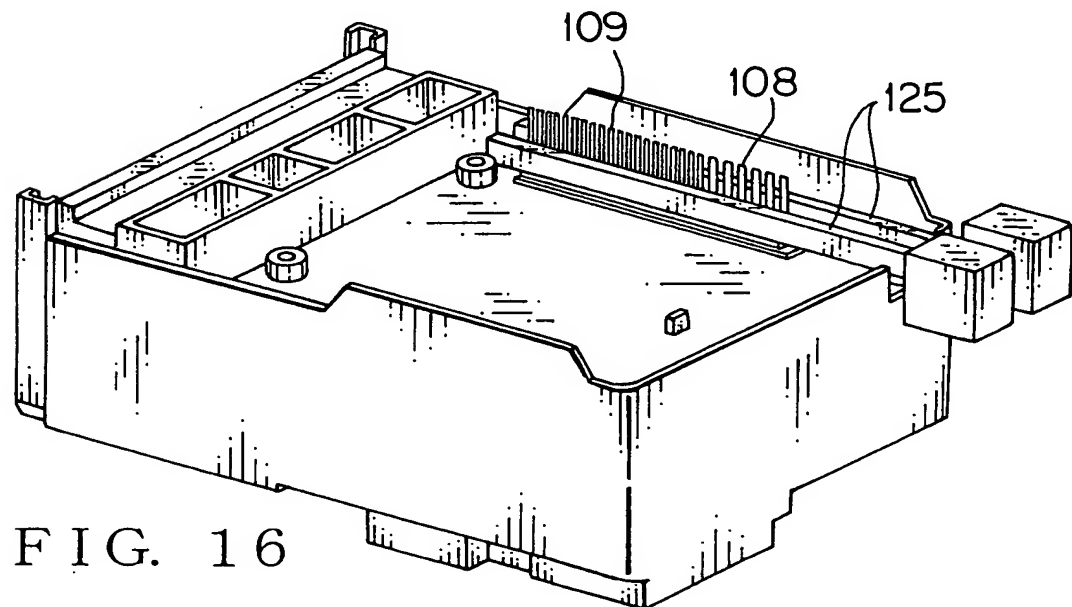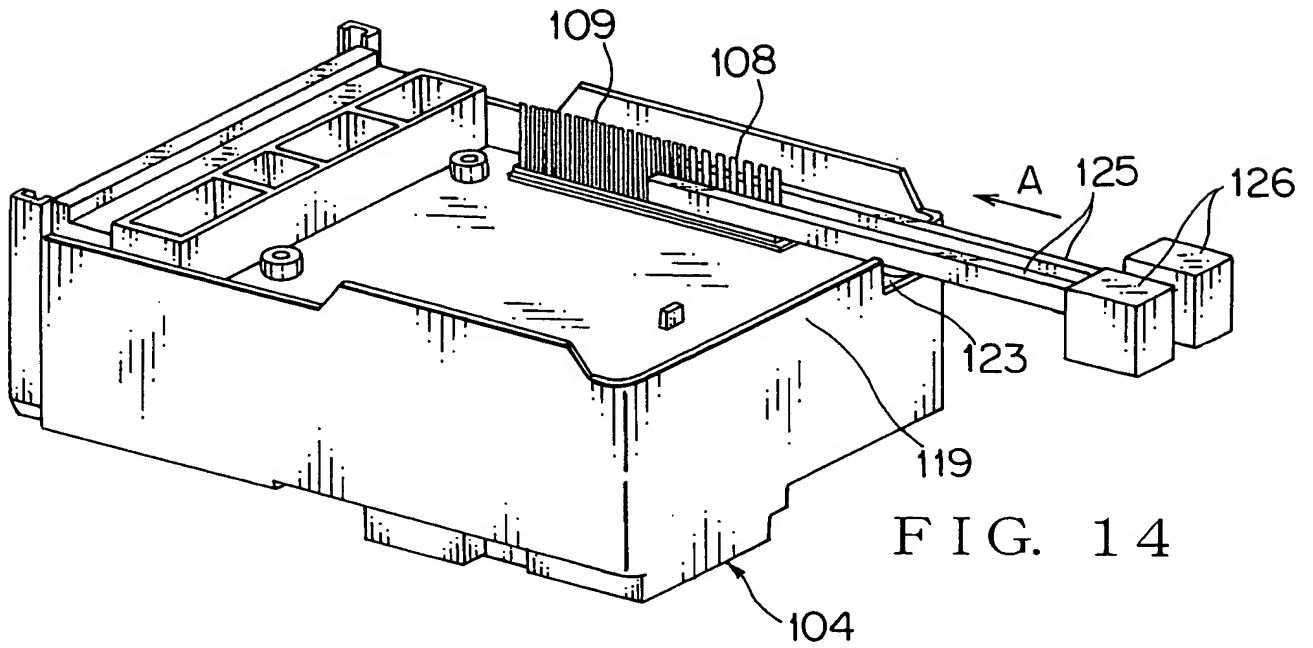

13/18

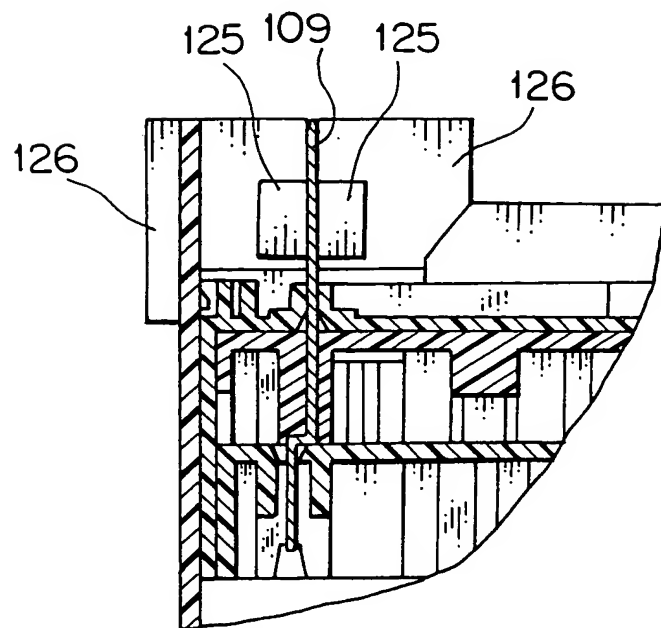


FIG. 17



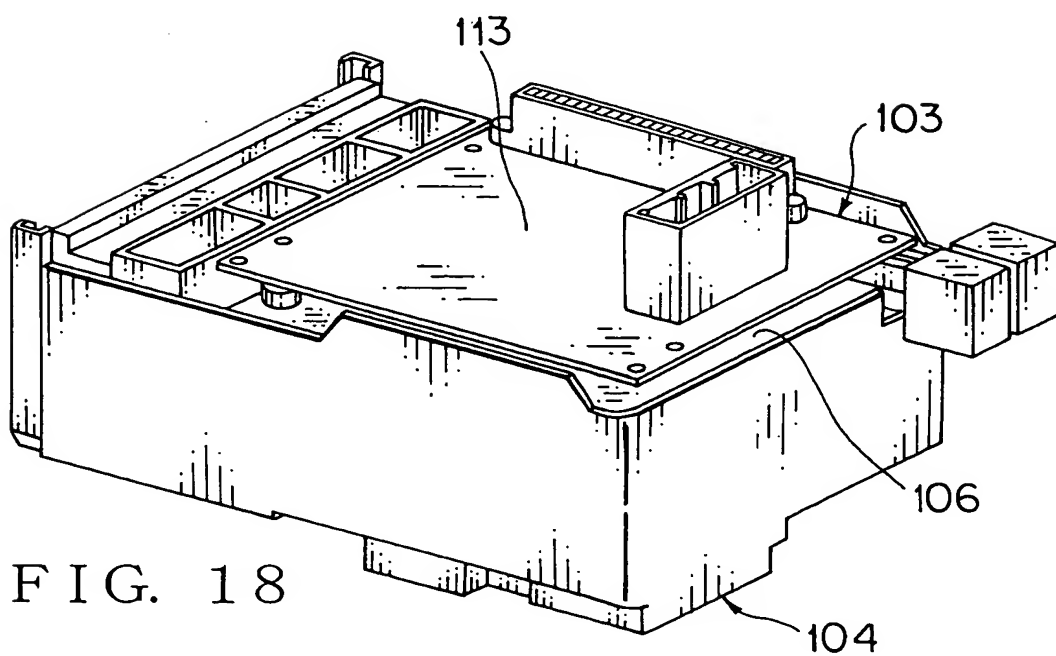


FIG. 18

14/18

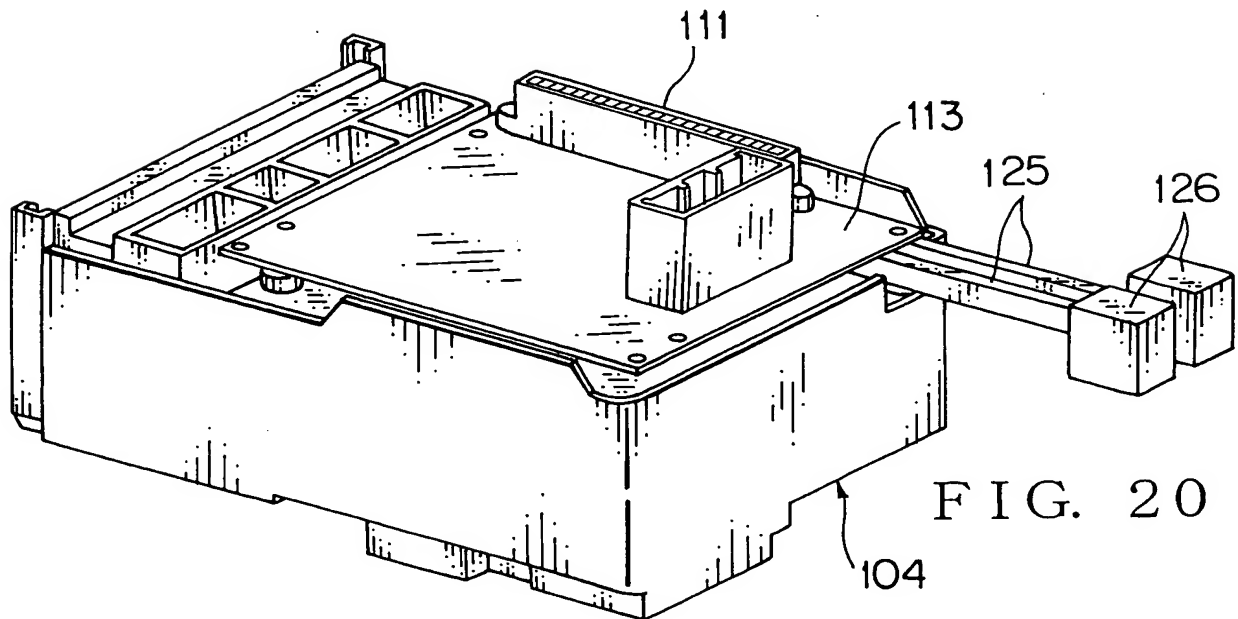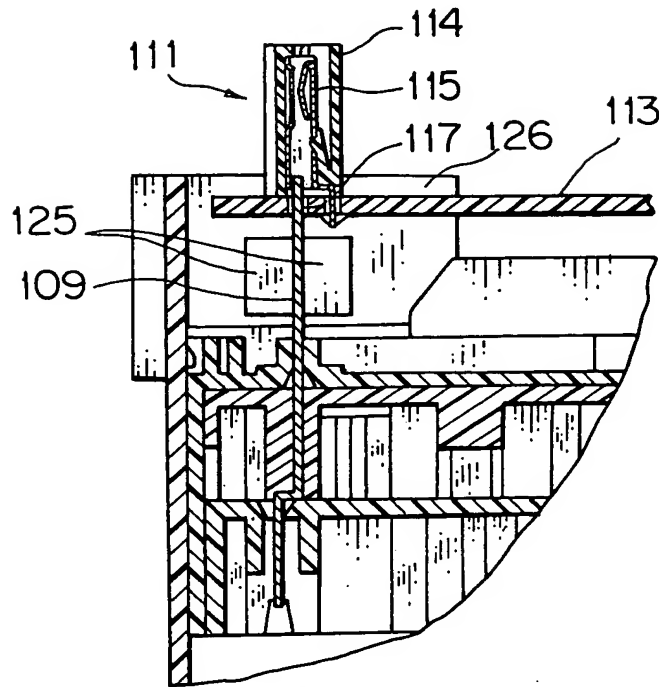

15/18

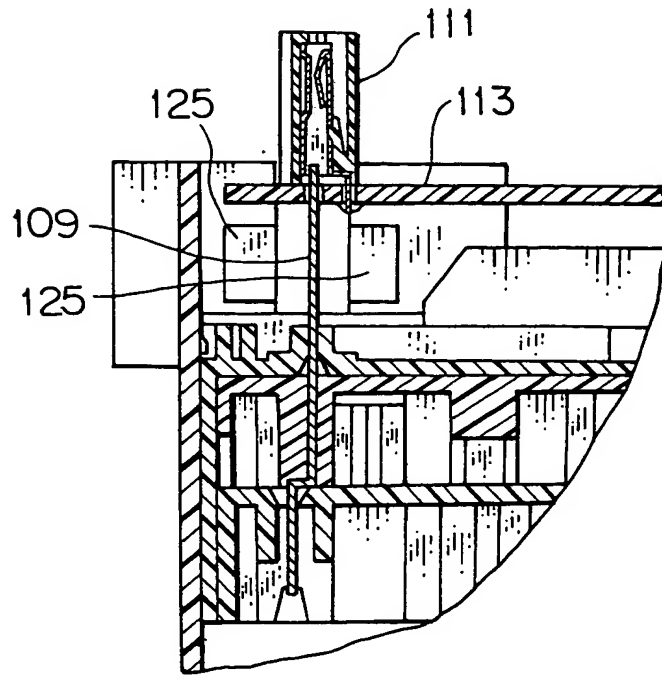


FIG. 21



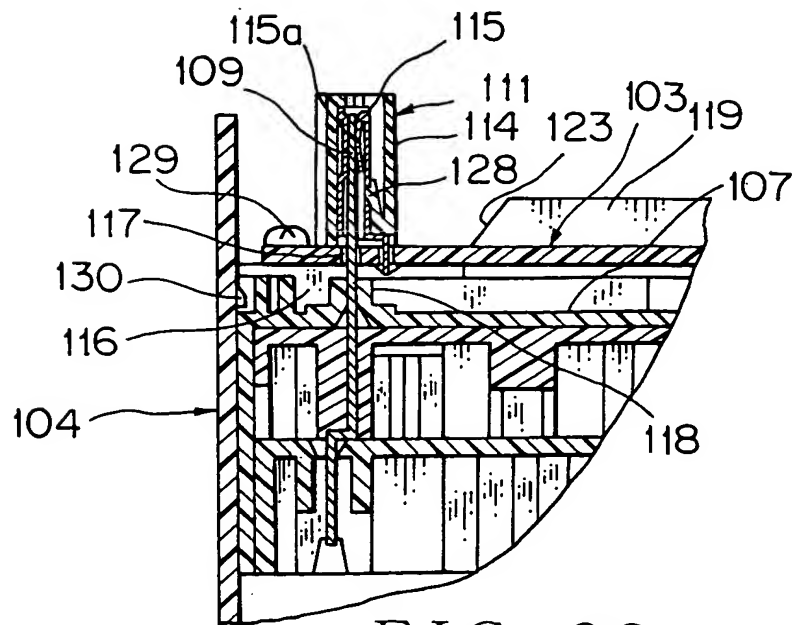


FIG. 23

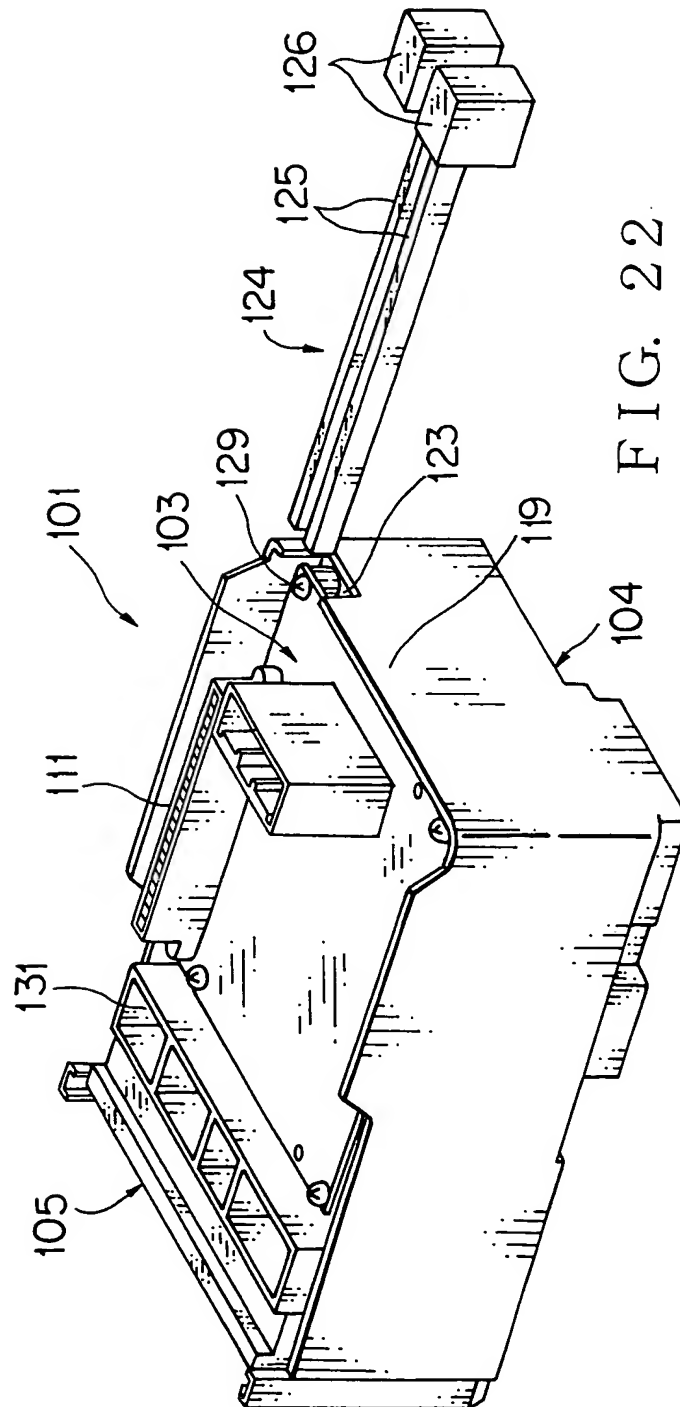

17/18

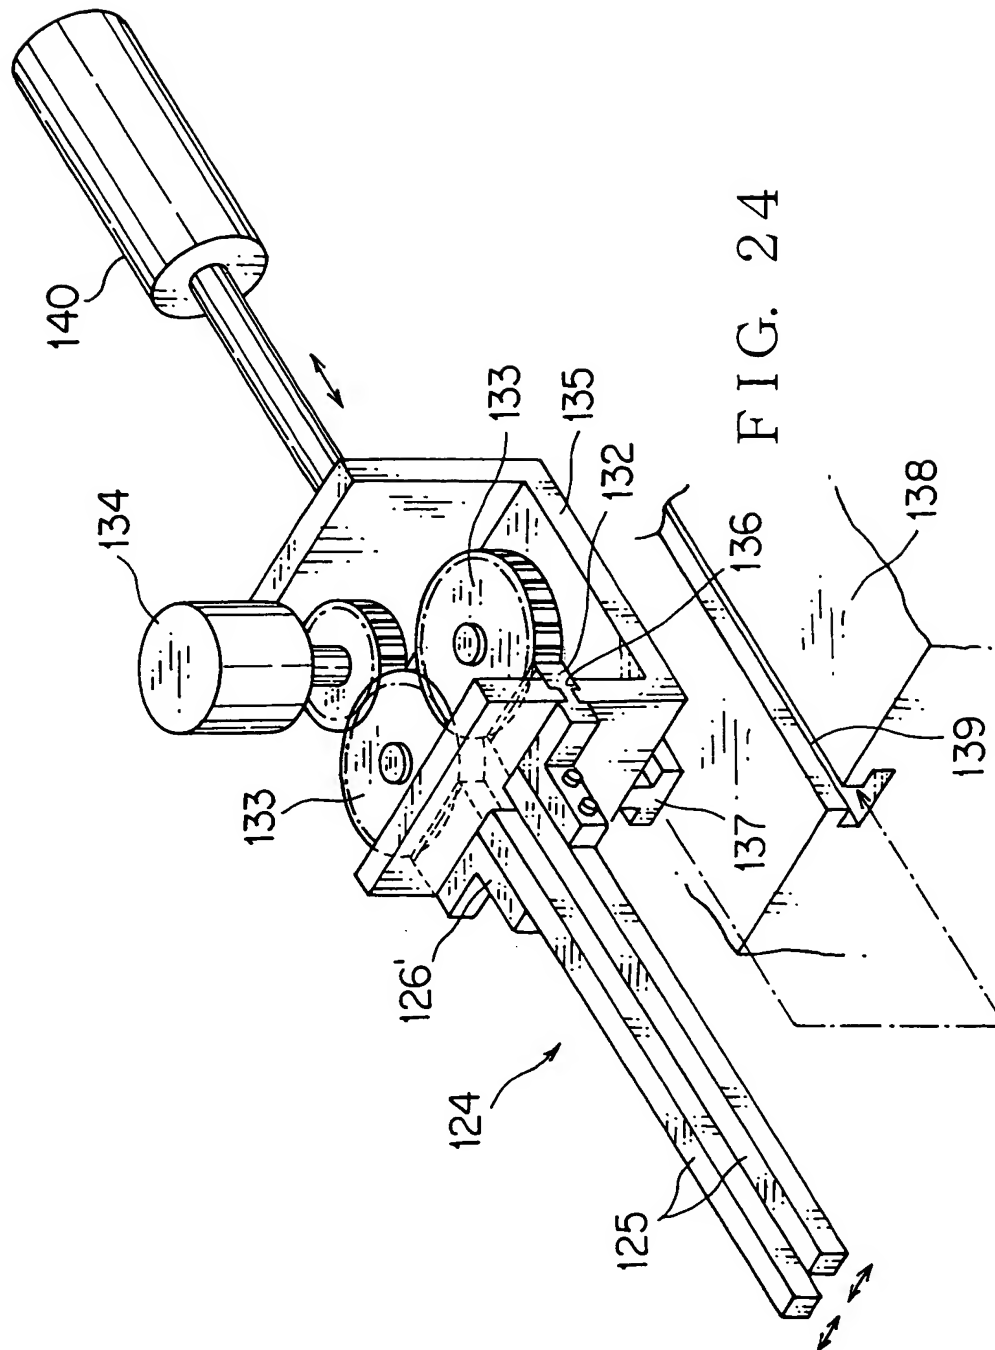

18/18

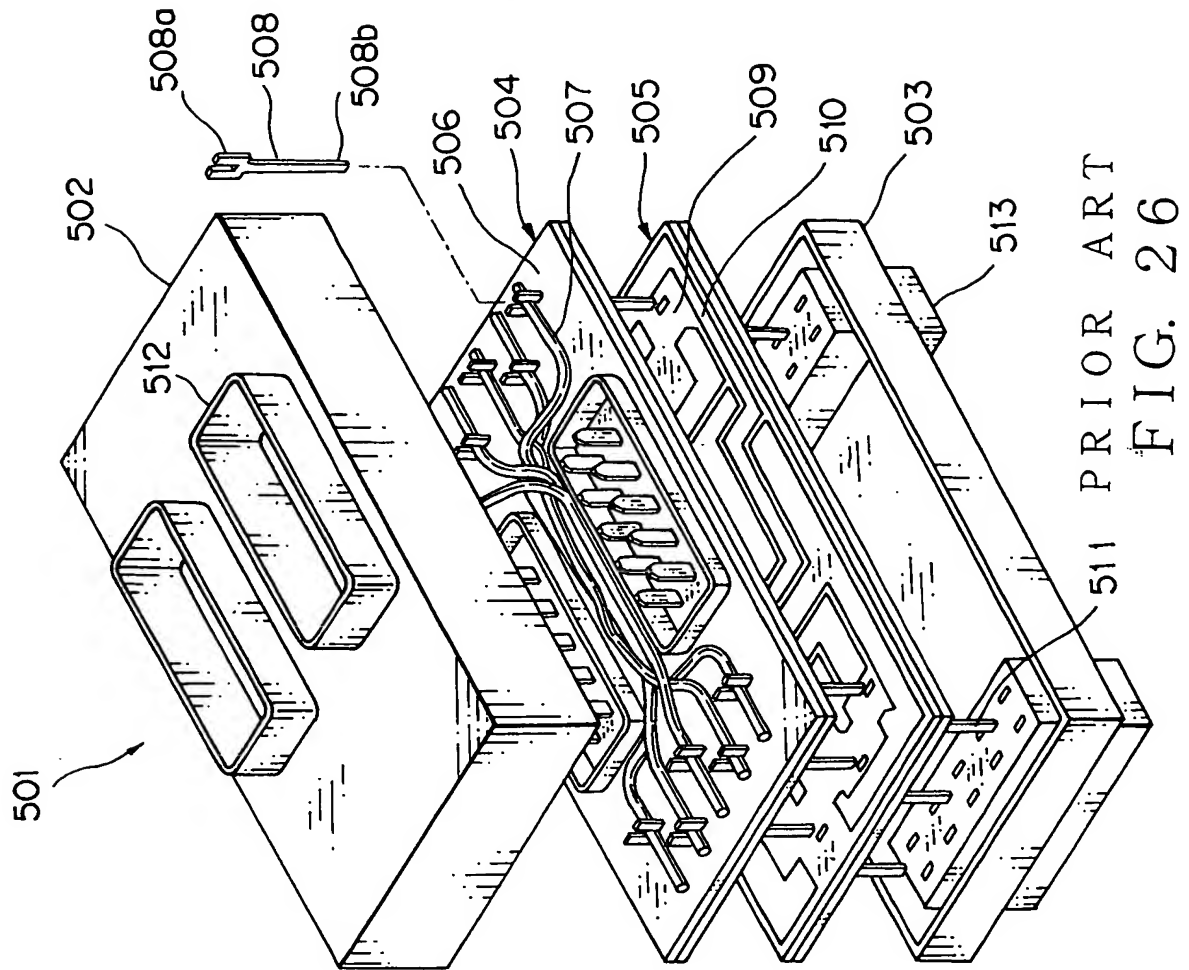


FIG. 26
 PRIOR ART

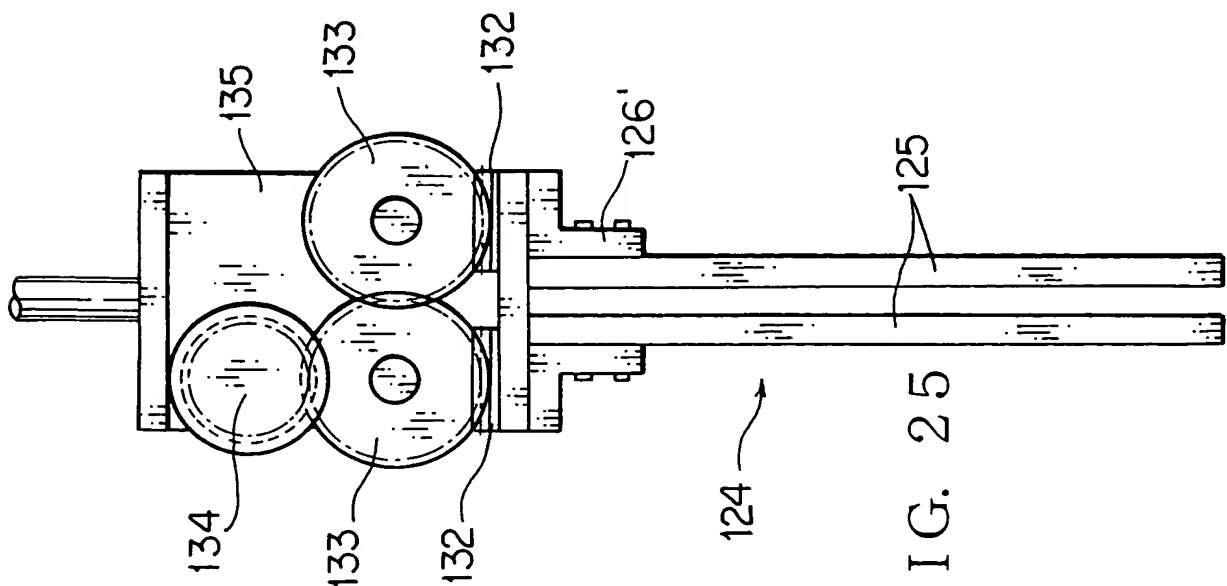


FIG. 25